




R. M. Young Company
Barometric Pressure Sensor Calibration Record
Serial Number: BPA14707
Calibration Date: November 30, 2023

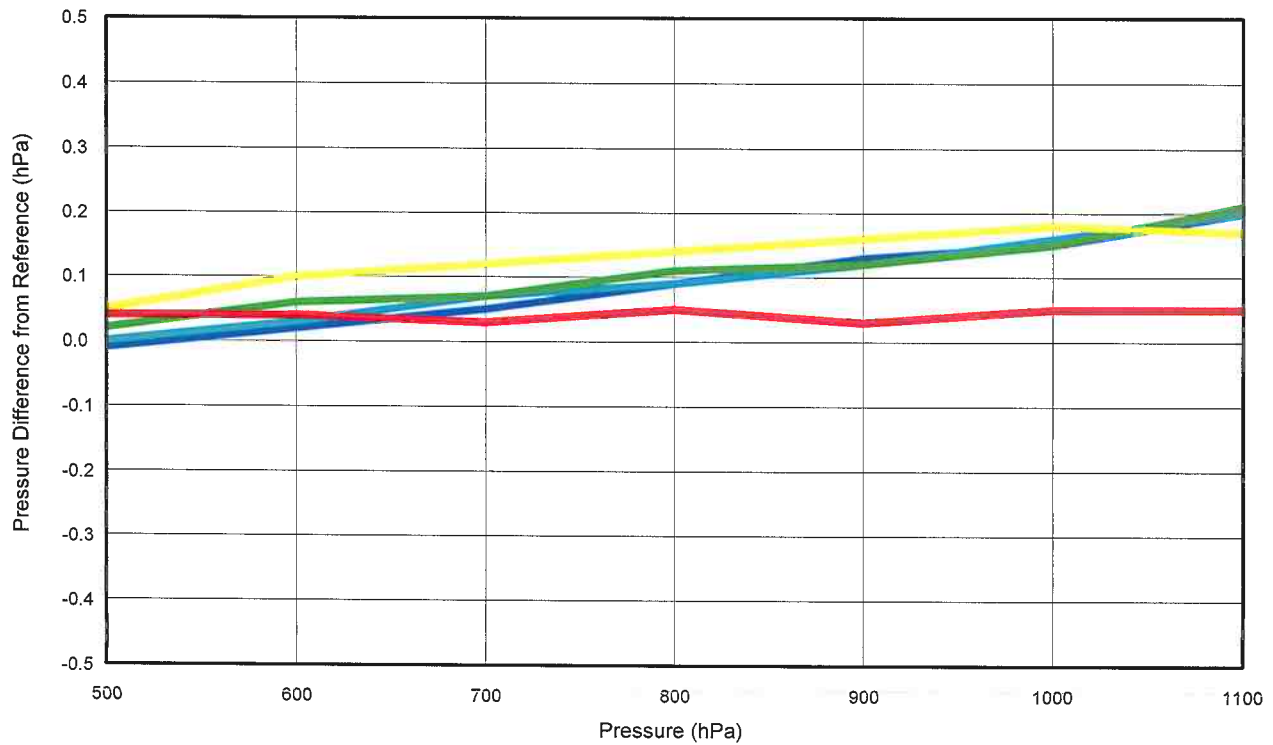

LEGEND:

- 40°C
- 25°C
- 0°C
- 25°C
- 60°C

Sensor calibration checked from 500 to 1100 hPa in 100 hPa increments at 5 temperatures.
Pressure reference traceable to NIST.

Average Difference from Pressure Reference: 0.09 hPa
Standard Deviation: 0.06 hPa